

QUICK START GUIDE




Patents pending on Seek Scan System and Fixed Heat Source

**SEEK SCAN DOES NOT DIAGNOSE COVID-19 OR OTHER DISEASE, ILLNESS OR DISORDERS.
THE SYSTEM MEASURES SKIN TEMPERATURE AS A PROXY FOR BODY TEMPERATURE.**

TABLE OF CONTENTS


What's In The Box.....	2
System Setup.....	3
Software Overview.....	4
Settings & About Menu.....	5
Tips For Optimal Performance.....	6
Regulatory.....	7




WHAT'S IN THE BOX




SYSTEM SETUP




1. Connect USB stick to PC or tablet and follow instructions to install Seek Scan software.




2. Place two pieces of tape 5 feet apart. Distance is critical to system performance.




3. Set tripod heights to 5 feet. Tripods not included.



4. Heat source automatically turns on once plugged in. Ready when light stops blinking.






5. Attach camera to tripod and connect cable to PC or tablet. Software must be already installed.





6. Heat source and person should be 5 feet (1.5 meters) from the camera.


SOFTWARE OVERVIEW




1.  means the heat source is not detected.
 means no person is detected.




2. This shows the heat source is detected but no person  is detected.




3. Set a custom alarm by clicking up & down arrows. Switch from F to C in settings menu.



4. Blue box means the camera has detected a face and is measuring skin temperature.





5. Green box means estimated body temperature is below the alarm temperature.



6. Red box means estimated body temperature is above the alarm temperature.



SETTTINGS MENU

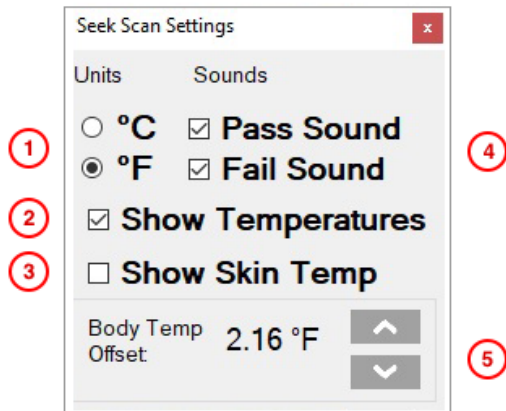

1. Change between Celsius and Fahrenheit.
2. Turn the temperature display on or off.
3. Seek Scan measures skin temperature as a proxy to estimate body temperature. Check this box to also show the skin temperature measurement.
4. Turn alert sounds on or off.
5. This allows the user to adjust the skin to body temperature offset for their own environment.

ABOUT MENU

1. Displays your version of Seek Scan Software.
2. Displays your camera's serial number. Enter this number when registering to activate your warranty.
3. Visit our support site to solve technical issues and receive support if needed.
4. It is important to register your product to activate your warranty and receive the latest product information from Seek Thermal.

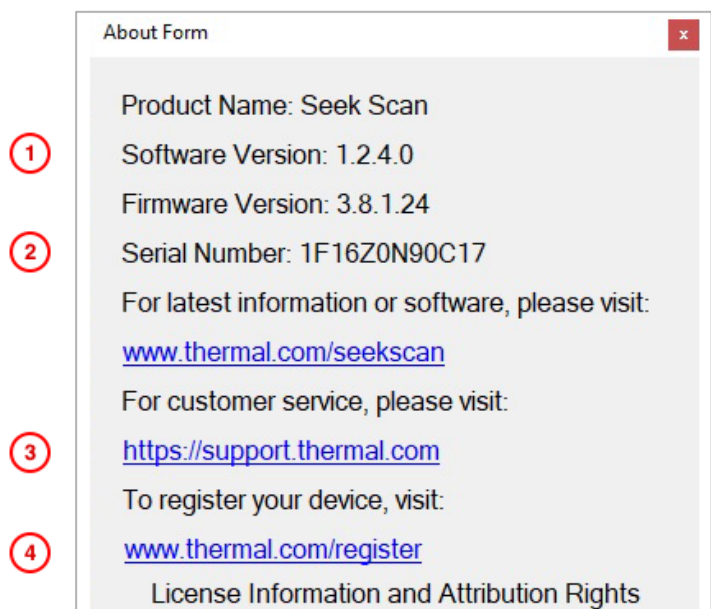

TIPS FOR OPTIMAL PERFORMANCE

1. Subjects should look directly at the camera during measurement.
 2. Set up your screening area with the camera pointed at the Heat Source in front of a wall. This will help create a flat thermal background and allow for faster scan times and more reliable readings. Warm objects in the background that are near a person's skin temperature or warmer than 40°C (104°F) may reduce system performance.
 3. After set up, measure and confirm the distance from the Heat Source to the Camera is no further than 5 feet (1.5 meters).
 4. We recommend marking the ground with tape or floor decals to ensure all subjects are measured from the exact same distance and while positioned directly next to the Heat Source.
 5. For more consistent readings, ensure the subject's eyes are clearly exposed by removing any eyewear. Subjects wearing a face mask should pull it down slightly and subjects wearing a hat should lift the brim to fully expose the eyes.
-

SKIN TEMPERATURE VS BODY TEMPERATURE

Seek Scan measures skin temperature as a proxy for body temperature.

Here are a few things to know about skin temperature measurement:

- Skin temperature is typically a few degrees less than body temperature. Similar to an infrared temporal thermometer, Seek Scan uses skin temperature to provide an estimated body temperature.
- Seek Scan is programmed to measure the most reliable parts of the face to produce the best results with high accuracy.
- A person's skin temperature may vary based on a variety of circumstances such as ambient temperature, sweat and eyewear. For this reason, Seek Scan is intended for indoor use only and in environmentally controlled rooms.

REGULATORY

FCC: This equipment has been tested and found to comply with the limits for a Class A digital device, pursuant to part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference when the equipment is operated in a commercial environment. This equipment generates, uses, and can radiate radio frequency energy and, if not installed and used in accordance with the instruction manual, may cause harmful interference to radio communications. Operation of this equipment in a residential area is likely to cause harmful interference in which case the user will be required to correct the interference at his own expense. Note: Any changes or modifications not expressly approved by the Seek Thermal Inc. could void the user's authority to operate the equipment.

WEEE: This symbol on the product(s) and / or accompanying documents means that used electrical and electronic equipment should not be mixed with general household waste. For proper treatment, recovery and recycling, please take this product(s) to designated collection points where it will be accepted free of charge. Alternatively, in some countries, you may be able to return your products to your local retailer upon purchase of an equivalent new product. Please contact your local authority for further details of your nearest designated collection point. Penalties may be applicable for incorrect disposal of this waste, in accordance with you national legislation.

ROHS: This RoHS-compliant product conforms to the European Union Restriction of the Use of Certain Hazardous Substances (RoHS) in Electrical and Electronic Equipment. Seek Thermal Inc. ensures RoHS conformance by requiring supplier Declarations of Conformity, monitoring incoming materials, and maintaining manufacturing process controls.

Industry Canada: This Class A digital apparatus complies with Canadian ICES-003. Cet appareil numérique de la classe A est conforme à la norme





thermal.com